

FLAT KNIT CUSTOM ORDERS

VenoTrain® curaflow



221

Hospital

221

Customer name: _____ Customer no.: _____

Contact: _____

Order date: _____ Previous order no.: _____

Patient name: _____

Quotation Order

Signature/Company stamp: _____

Leg

Colors Cream Caramel Black
 Anthracite Navy Bordeaux
 Royal Orange

Compression Ccl1 Ccl2 Ccl3 Ccl4
 Left leg
 Right leg
 Panty area

Quantity Pair _____ One piece _____

The colors cream, caramel and black are available for hospital supply.

Stockings: AD AG
 Leg piece _____

Edging:
 Silicone dotted band
 Wide (4.7 cm)
 Narrow (2.5 cm)
 Garter belt
 Striped silicone top band
 Laterally slanted edging
 Leg elevation at the front

Pantyhose: Pantyhose AT
 Maternity pantyhose ATU
 Single-leg pantyhose ATE
 Leggings BT
 Legging B1T
 3/4 length CT
 Above-knee pantyhose ET
 Cycling shorts FT
 Two-part

Waist edging:
 Silicone dotted band
 Waist band
 Edging with compression
 Loop/pull-through elastic

Additional features:
 Without knee zone/knee ellipse
 Zip fastening*
 Lining**
 Top band, inside* Wide (4.7 cm)
 Narrow (2.5 cm)



Women's gusset:
 Standard Open
 Compressive

Men's gusset:
 Standard With fly
 Compressive

* Length and position given in special requests

All sizes in cm. The purchaser is responsible for ensuring that all size information is correct. Custom-made products are non-returnable.

Special requests: _____

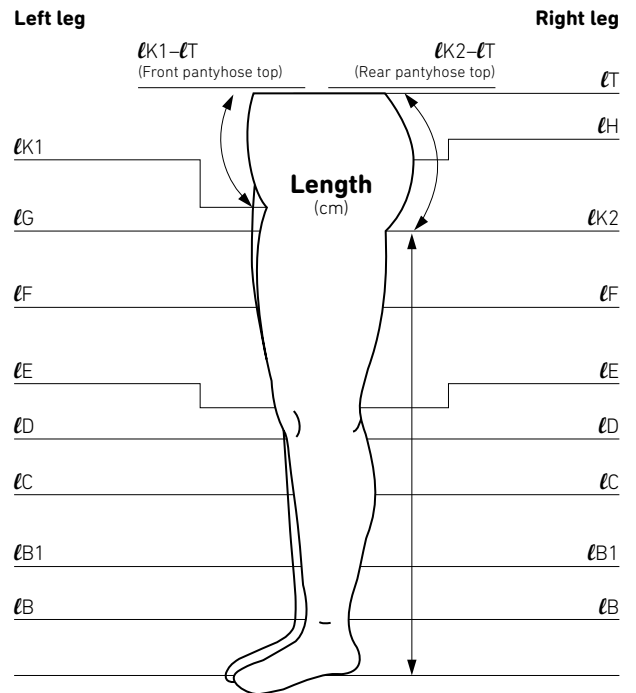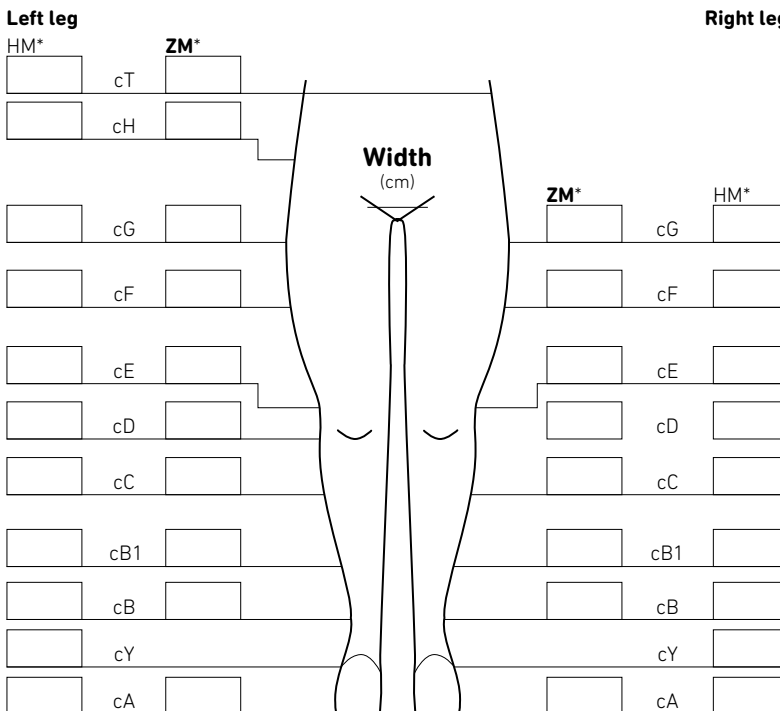

* HM = Measurement next to the skin | ZM = Measurement with tape tightened

Pressure pad: Left Right Medial Lateral

Lymph pad: Foam Silicone Pocket only

Dimensions for pressure pad
 Left: P1 _____ cm P2 _____ cm
 Right: P1 _____ cm P2 _____ cm

Provisional seam

Hallux Left Right

Anatomical foot
 Left Right
 cA1 _____ cm cA1 _____ cm
 lA1* _____ cm lA1* _____ cm

* is the length from the heel to measuring point cA1

Left foot **Foot** **Right foot**
 lA outside _____ Length _____ outside lA (cm)
 lAi inside _____ inside lAi
 lZ whole foot _____ whole foot lZ

Straight foot **Slanted foot**
 Open Open
 Closed Closed
 90° heel Instep widening